




湖北省计量测试技术研究院

Hubei Institute of Measurement and Testing Technology

证书编号: 鄂检校字(2019)第001号

Certificate No.

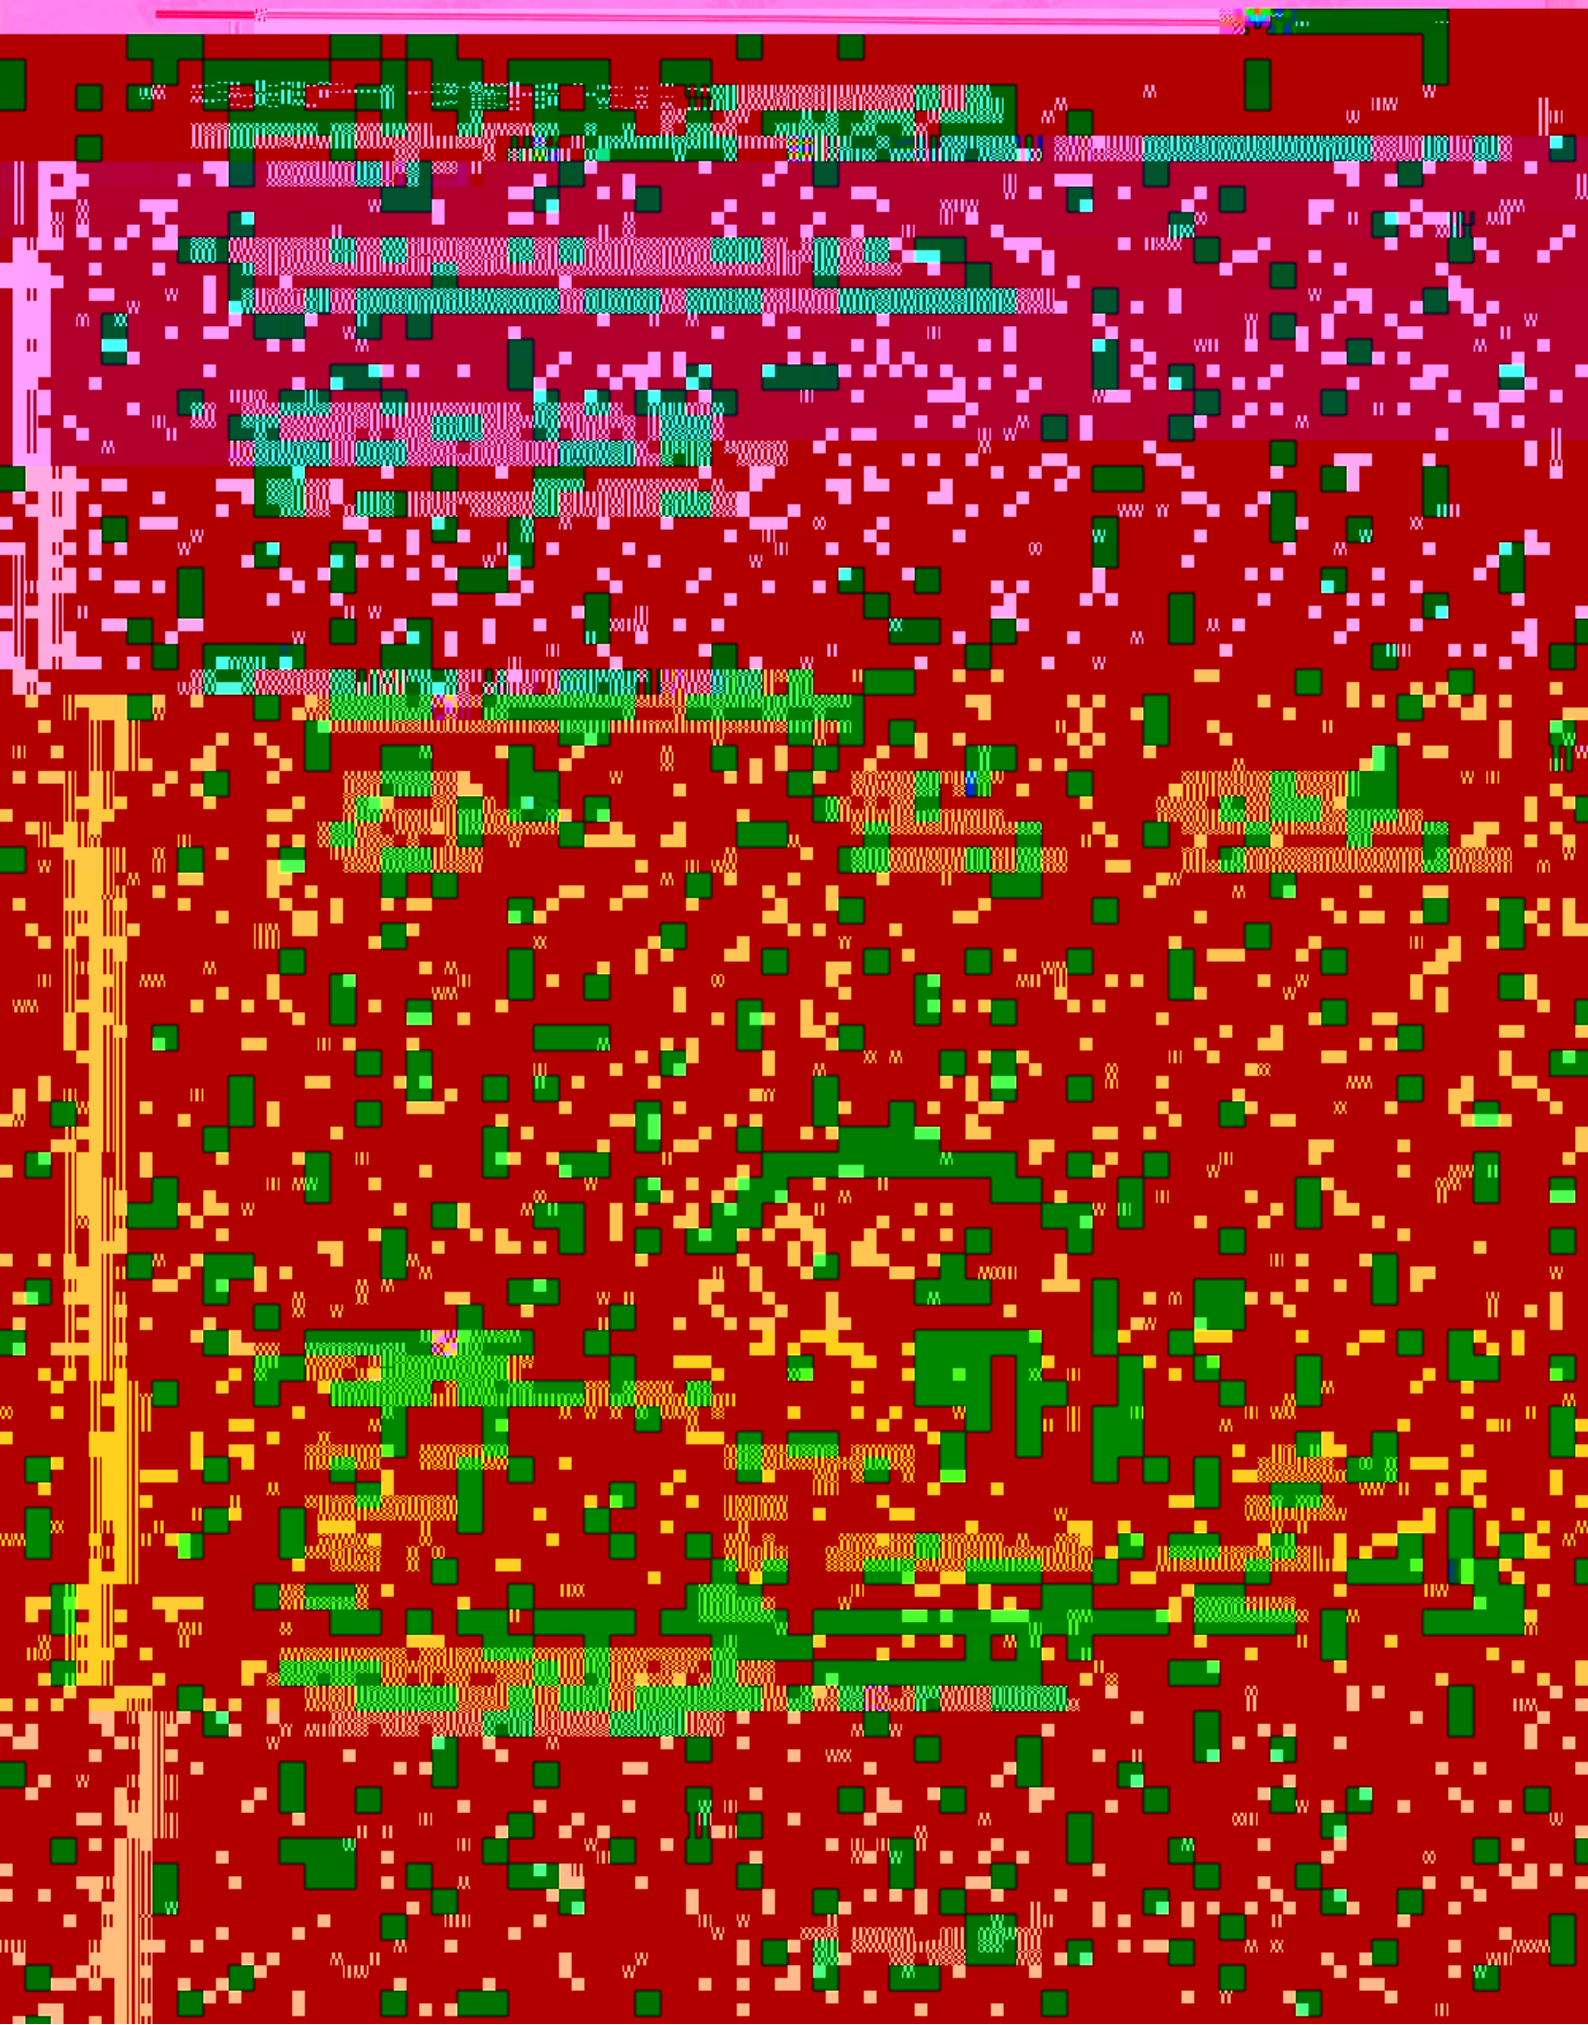

校准数据报告结果

Data/Results of Calibration

电压:									
被测输出 值(V) AC	标准表显示值(V) AC 50Hz				被测输出 值(V) DC	标准表显示值(V) DC			
	Ua	Ub	Uc	Urel (k=2)		Ua	Ub	Uc	Urel (k=2)
10.00	9.9971	9.9955	9.9962	0.09%	10.00	9.9967	10.001	9.9992	0.08%
50.00	49.977	49.967	49.973	0.09%	50.00	50.021	50.015	50.015	0.08%
80.00	79.956	79.941	79.949	0.09%	80.00	80.032	80.021	80.019	0.08%
100.00	99.942	99.920	99.932	0.09%	100.00	100.04	100.03	100.03	0.08%
120.00	119.91	119.90	119.91	0.09%	160.00	160.07	160.05	160.04	0.08%
电流:									
被测输出 值(A) AC	标准表显示值(A) AC 50Hz				被测输出 值(A) DC	标准表显示值(A) DC			
	Ia	Ib	Ic	Urel (k=2)		Ia	Ib	Ic	Urel (k=2)